

1/8

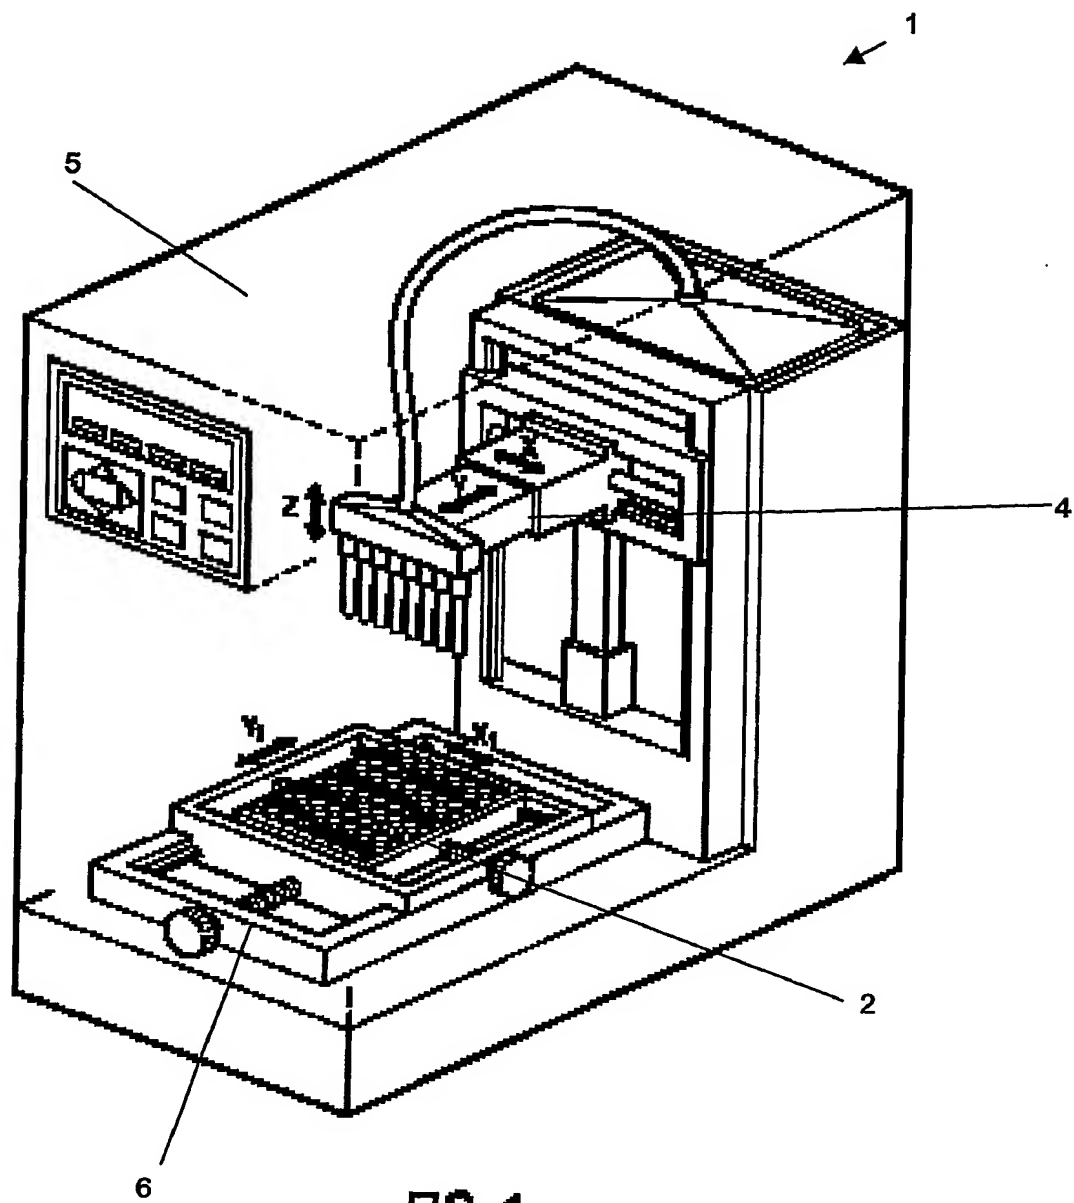


FIG. 1

2/8

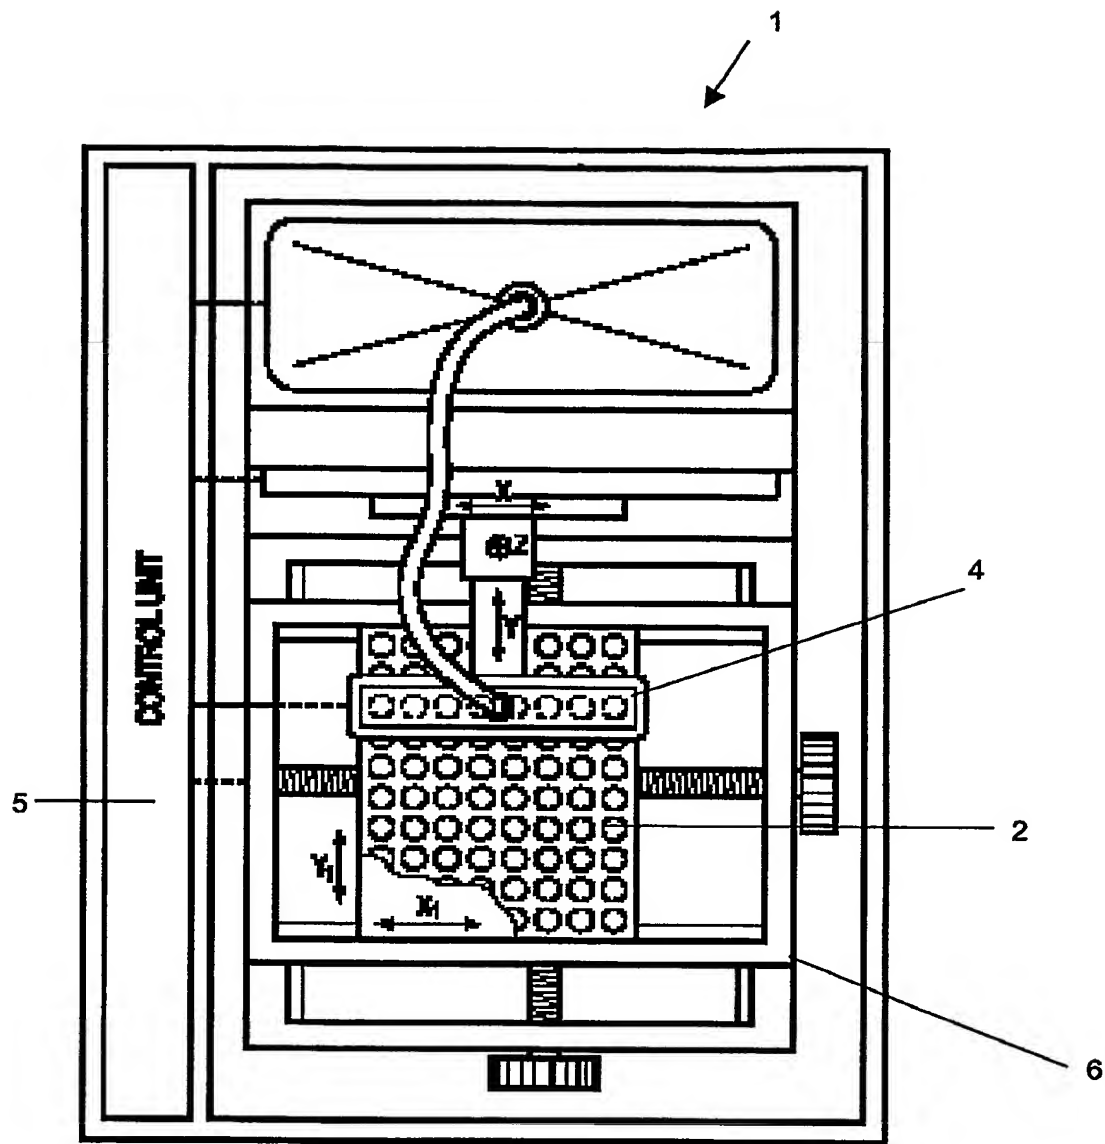


FIG. 2

3/8

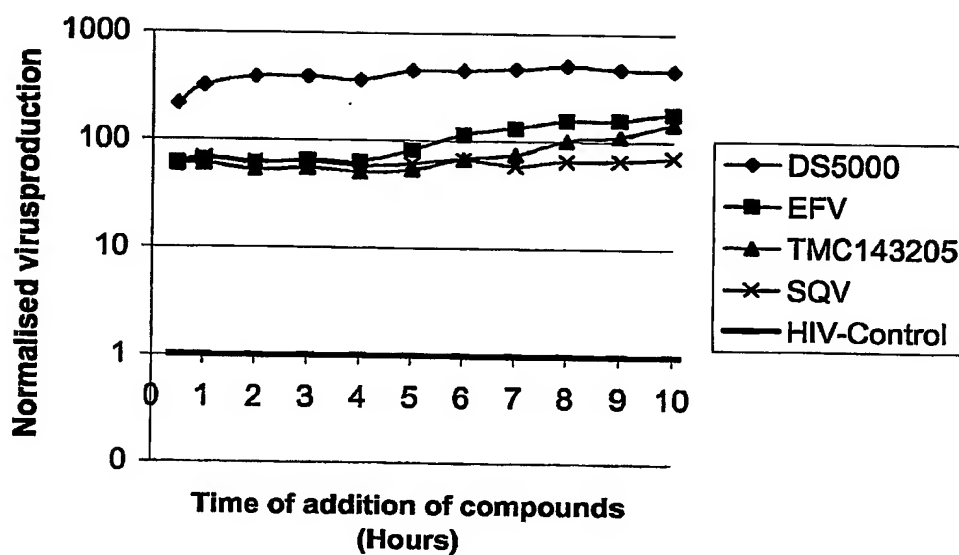


Figure 3

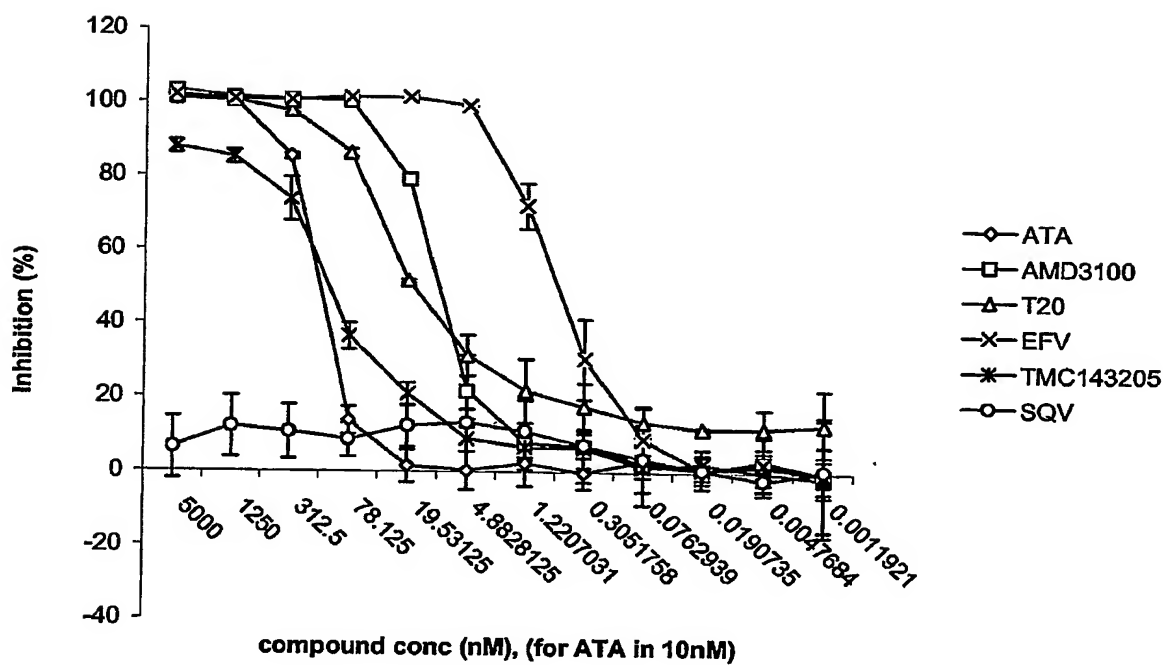


Figure 4

4/8

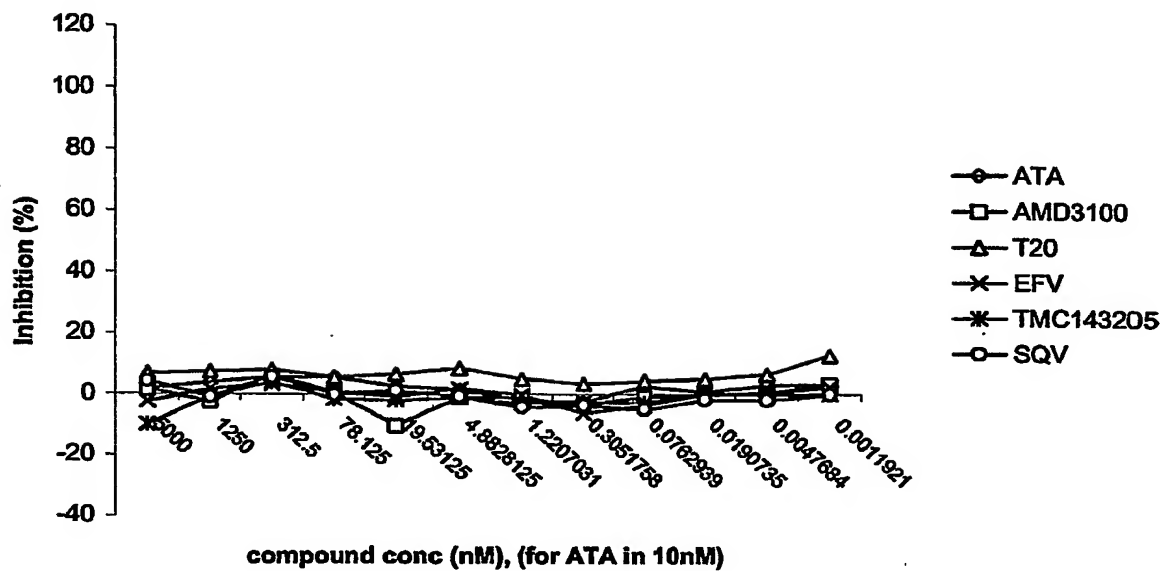


Figure 5

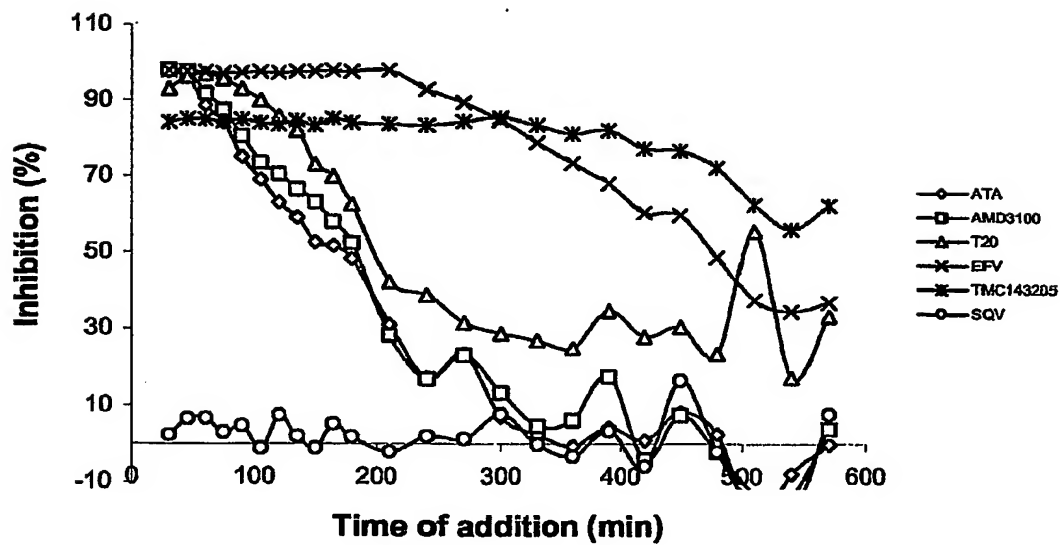


Figure 6

5/8

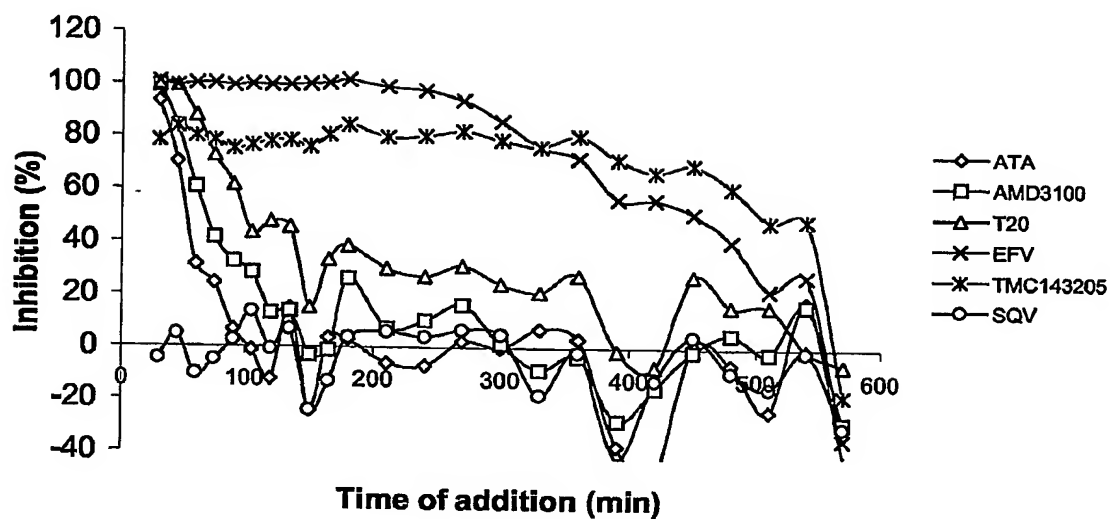


Figure 7

Time (min) 30 60 90 120 180 240 300 360 420 480 540 600

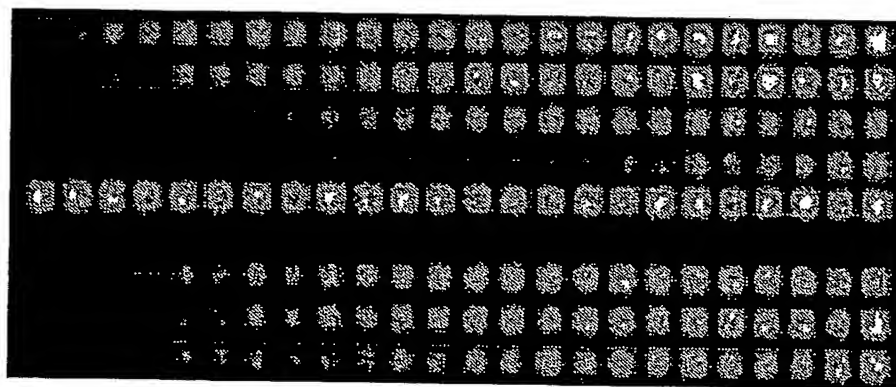


Figure 8

CD4-inhibitor
X4-inhibitor
Fusion-inhibitor
RT
Virus control
Cell control
Test-compounds

BEST AVAILABLE COPY

6/8

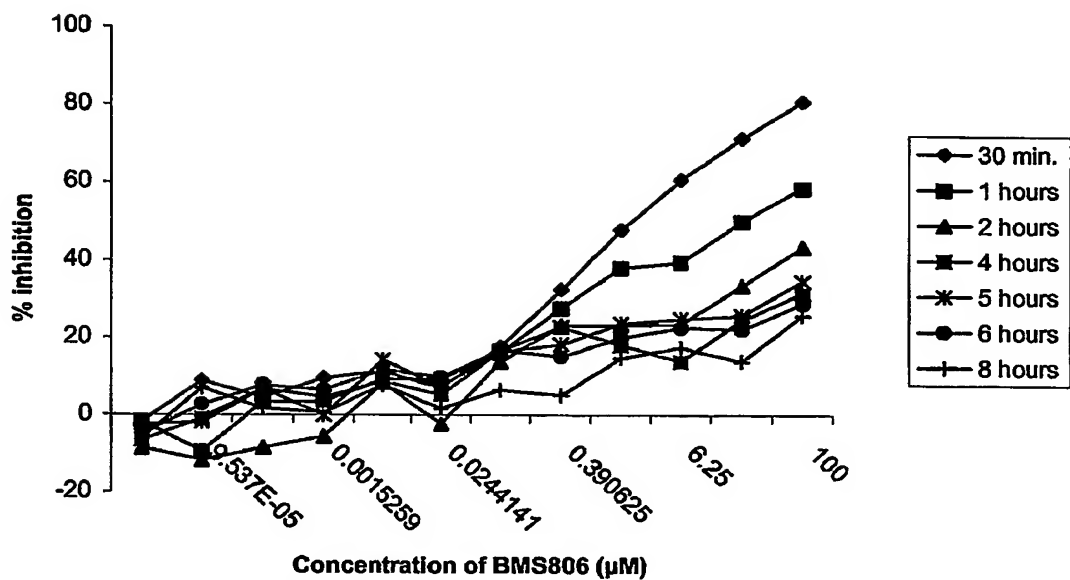
Anti-viral-experiment with TOA protocol: **23°C**

Figure 9A

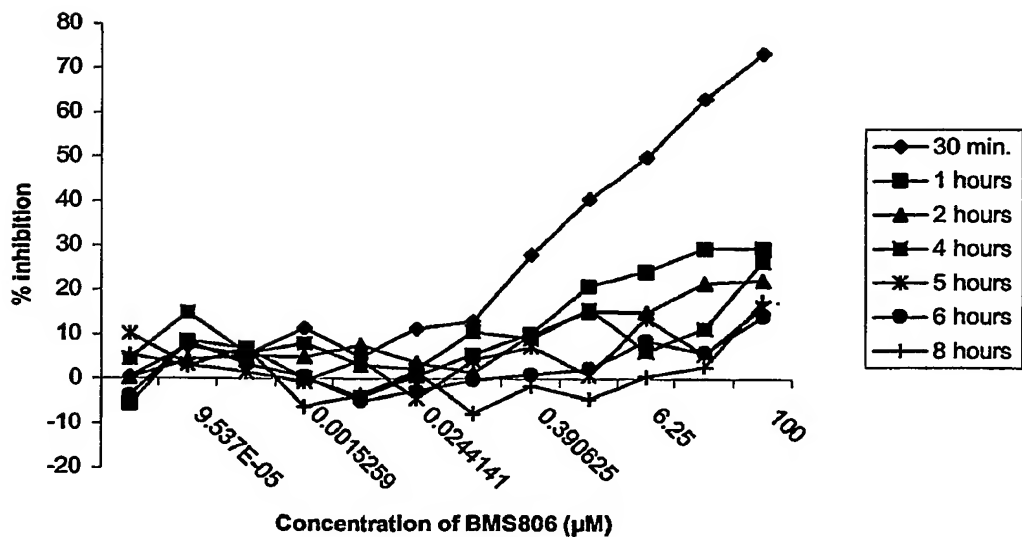
Anti-viral-experiment with TOA protocol: **37°C**

Figure 9B

7/8

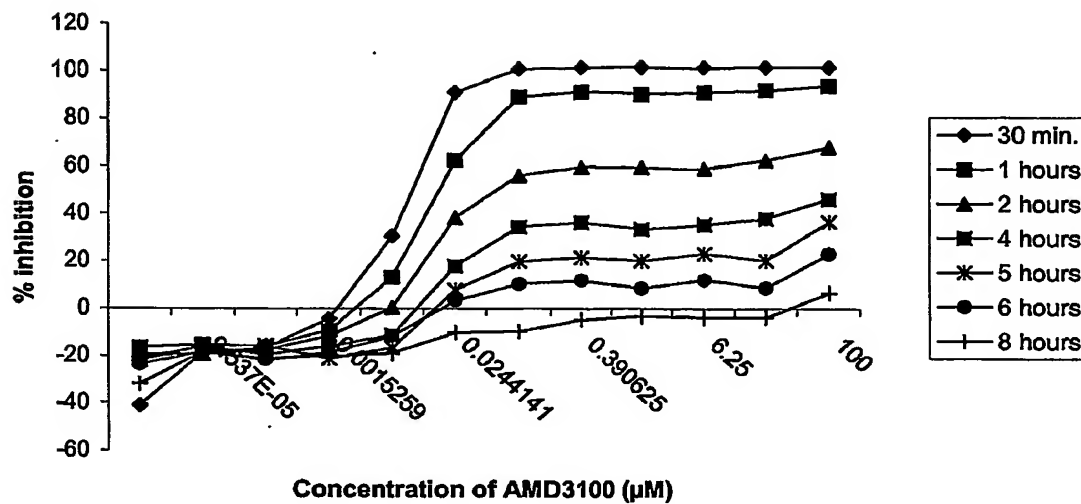
Anti-viral-experiment with TOA protocol: **23°C**

Figure 10A

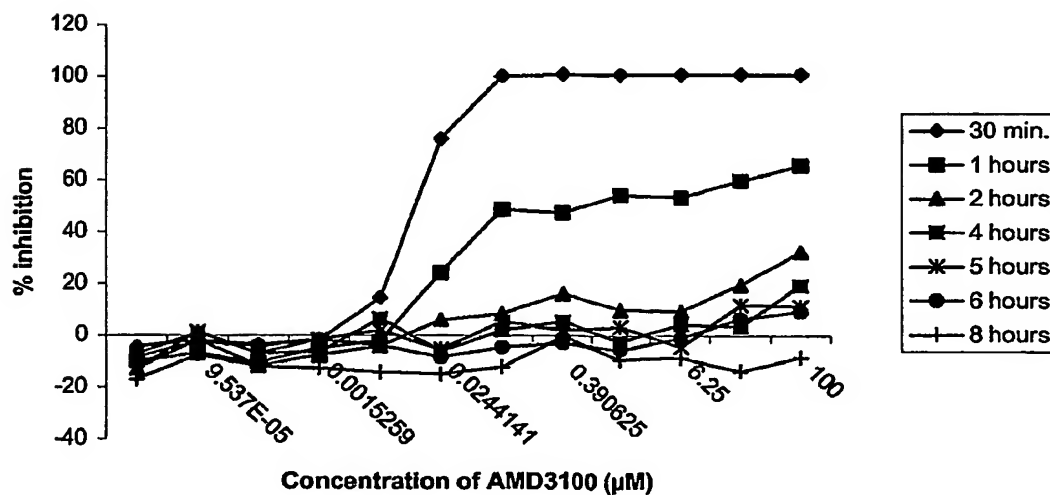
Anti-viral-experiment with TOA protocol: **37°C**

Figure 10B

8/8

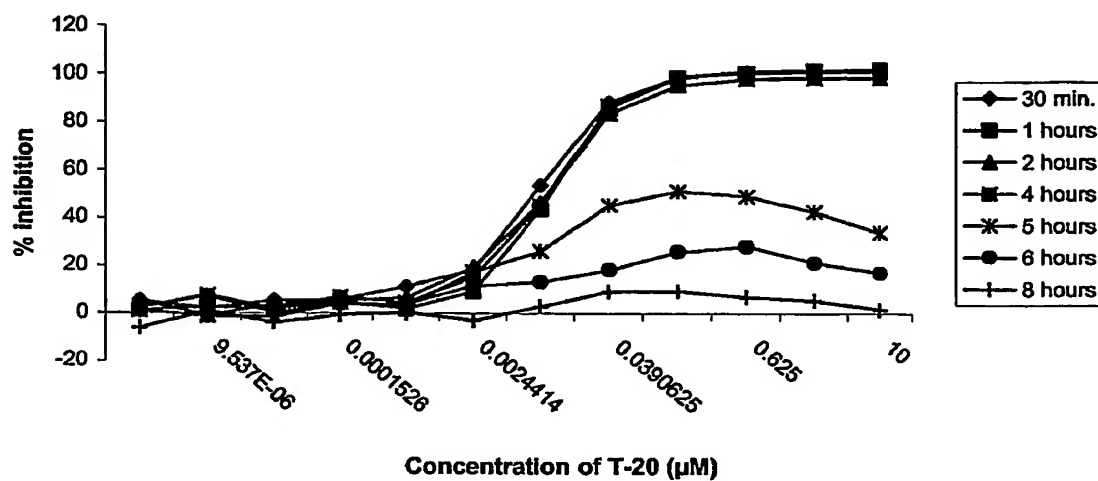
Anti-viral-experiment with TOA protocol: **23°C**

Figure 11A

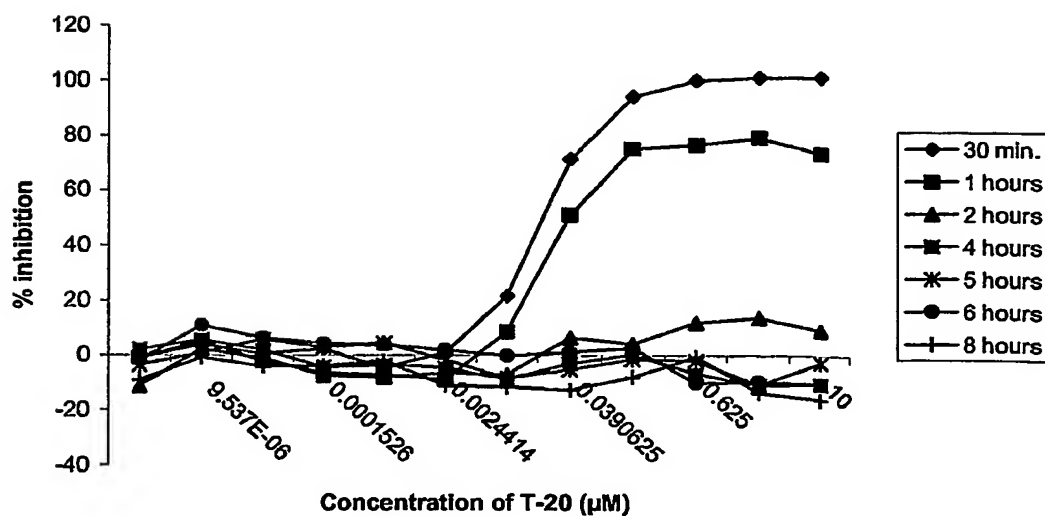
Anti-viral-experiment with TOA protocol: **37°C**

Figure 11B